

Setup


Logger: Omega OM-91 - New Device
Logger Start: Button Press
Logger Interval: 10 secs

Alarms

Temperature Logging: Enabled
Temperature Alarm (High): nan
Temperature Alarm (High): nan

Statistics

Temperature Maximum: 88.42 F
Temperature Minimum: 67.96 F
Temperature Average: 85.57 F
Temperature Samples: 2614

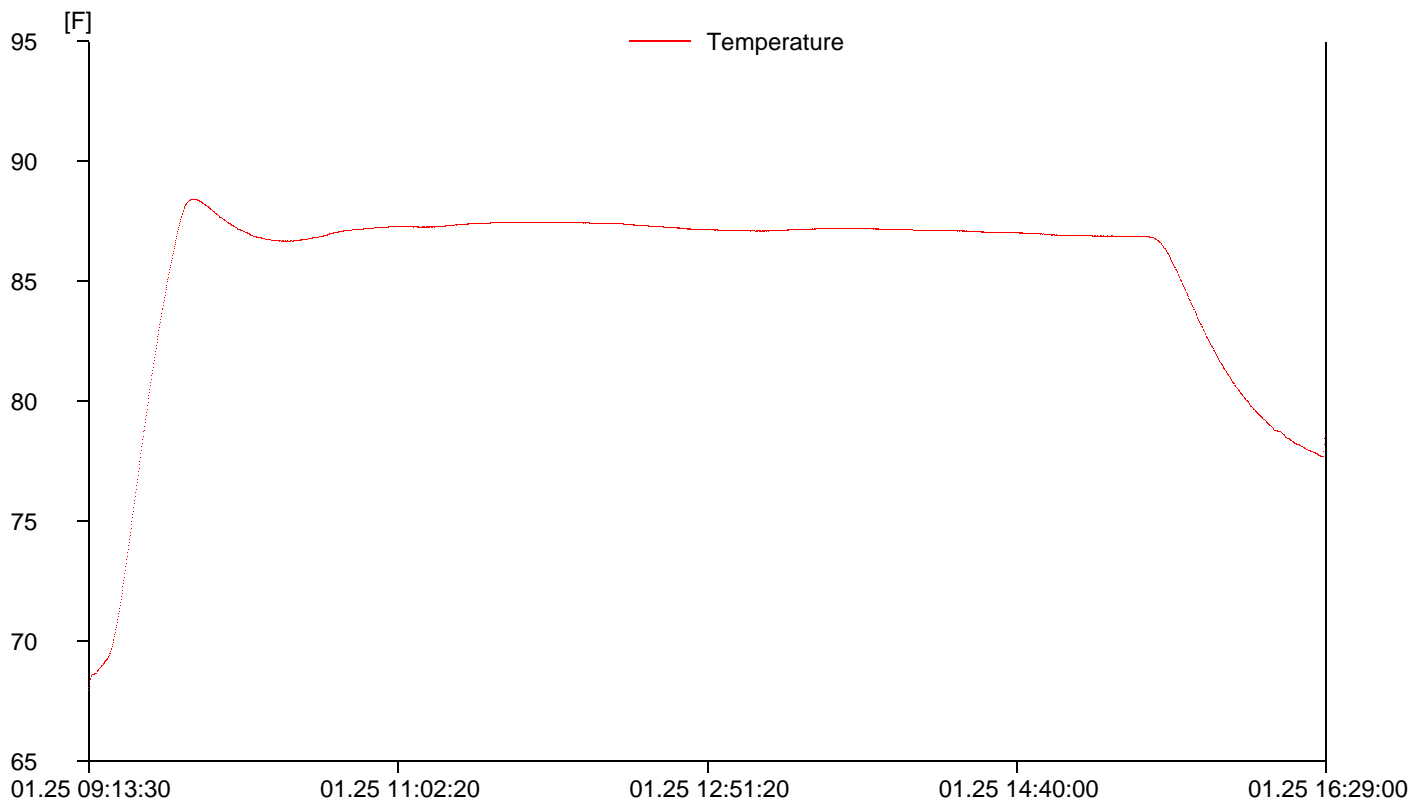

Pass/Fail

PASS. Logger within temperature limits.

Notes

DryBoost Test